

Regulation of Medical Devices in Hong Kong

Dr Terence CHEUNG
Principal Medical and Health Officer
Department of Health, Hong Kong SAR



衛生署

Department of Health

Content



衛生署
Department of Health

- Background
- Latest Legislative Development
- Medical Device Administrative Control System
 - Medical Device Listing
 - Safety Alerts and Adverse Incidents Reporting

Background




Medical Device Market in Hong Kong (1)



衛生署
Department of Health

- Hong Kong is a major hub for re-export of medical devices
Imported and locally manufactured medical devices

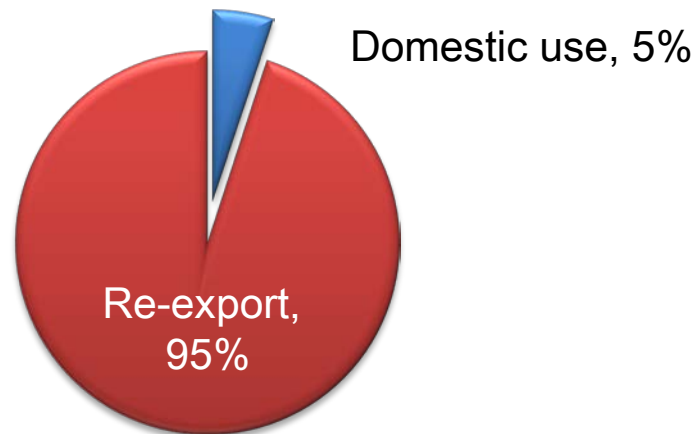

- It is estimated that there are
 - 50+ local manufacturers
 - 3 000+ medical device suppliers, including authorised representatives, importers and distributors

Source: BIA Report

Medical Device Market in Hong Kong (2)



衛生署
Department of Health

-
- | | |
|---------------------------|--|
| ■ Market Value | Estimated US\$ 300 million (2017) |
| ■ Market Size | ~ 40 000 medical devices <ul style="list-style-type: none">• including general medical devices and <i>in vitro</i> diagnostic medical devices (IVDMDs)• ~ 50% is Class I general medical devices |
| ■ Largest end-user | Hospital Authority (HA) <ul style="list-style-type: none">• accounts for approximately 70% - 90% of all the medical device purchased locally |
-

Source: BIA Report & Export.gov

Latest Legislative Development



衛生署

Department of Health

Regulation of Medical Devices



衛生署
Department of Health

- Currently, there is **no specific legislation** that regulates the manufacture, import, sale and use of medical devices in Hong Kong
- Other related legislations

Radiation Ordinance (Cap 303)

Pharmacy and Poisons Ordinance (Cap 138)

Undesirable Medical Advertisements Ordinance (Cap 231)

Consumer Goods Safety Ordinance (Cap 456)

Telecommunications Ordinance (Cap 106)

Medical Device Legislative Progress



衛生署
Department of Health

Statutory Regulation of Medical Devices

2019 Listing of Class B/C IVDMDs
(anticipated)

2018 Refined Legislative Proposal Focusing on
Pre-market and Post-market control of MD

2015 Listing of Distributors

2015-2016 Consultancy Study on the Control
of Use of Selected MD

2009 Listing of Class D IVDMD

2011-2013 Business Impact Assessment

2007 Listing of Local Manufacturers and Importers

2007-2008 Regulatory Impact Assessment

2006 Recognition of Conformity Assessment Bodies

2005 Listing of Class II/III MD

2003 Proposed Regulatory Framework
comprising Pre-market Control, Post-market
Control and Control on Use of High-risk MD

2004 Listing of Class IV MD

Medical Device Administrative Control System


2003 Public Consultation

Latest Regulatory Framework



衛生署
Department of Health

Focus on pre-market control and post-market control

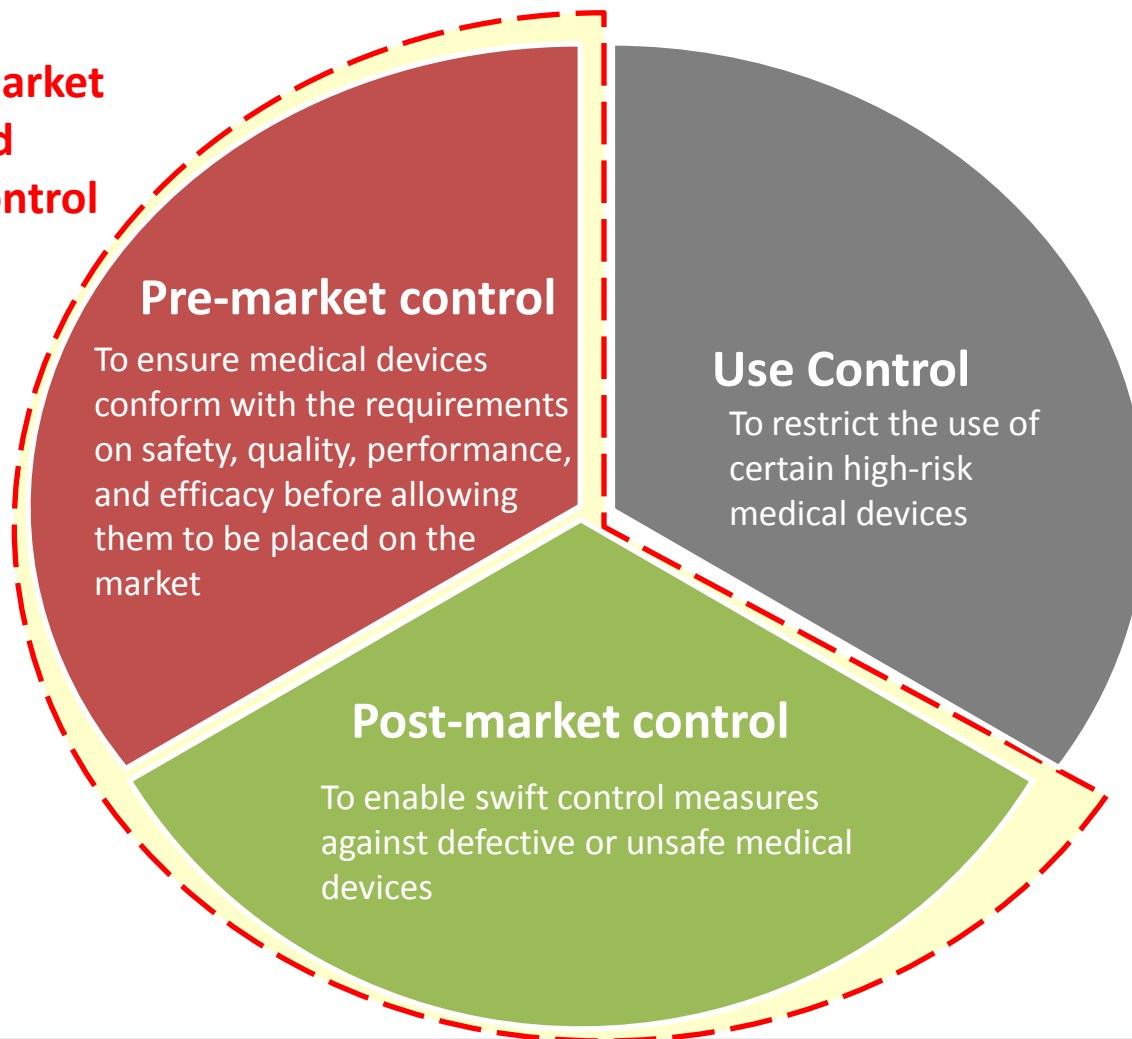

Medical Device Administrative Control System (MDACS)



衛生署

Department of Health

Medical Device Administrative Control System (MDACS)



衛生署
Department of Health

- Voluntary
- Adopting a risk-based approach recommended by **Global Harmonization Task Force (GHTF)**
- Taking into account local situations




IMDRF International Medical
Device Regulators Forum





Aims of MDACS

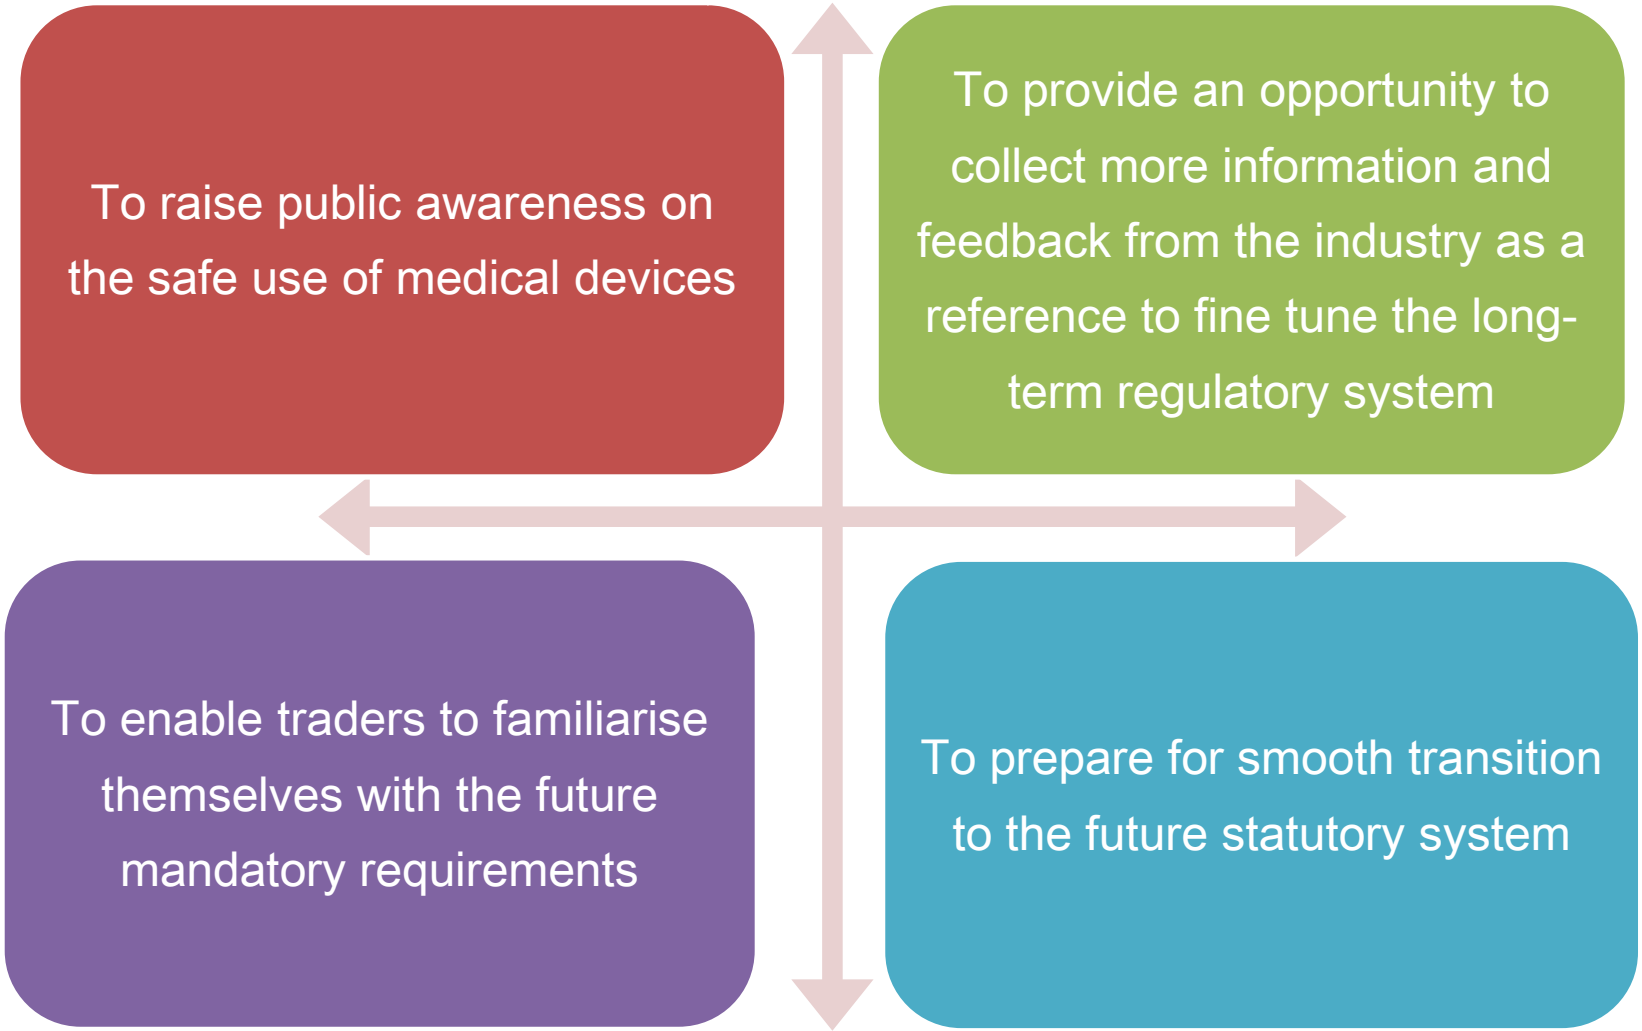

Current MDACS



衛生署
Department of Health

Medical Device Administrative Control System (MDACS)

Pre-market Control

Post-market Control

Listing System

1. Medical Device Listing
 - General medical devices (Class II, III, IV)
 - IVDMDs (Class D)
2. Trader Listing
 - Local Responsible Person (LRP)
 - Local manufacturer
 - Importer
 - Distributor

Conformity Assessment Bodies (CAB) Recognition Scheme


Medical Device Safety Alerts System & Adverse Incidents Reporting System



Medical Device Listing




Medical Device Listing Routes

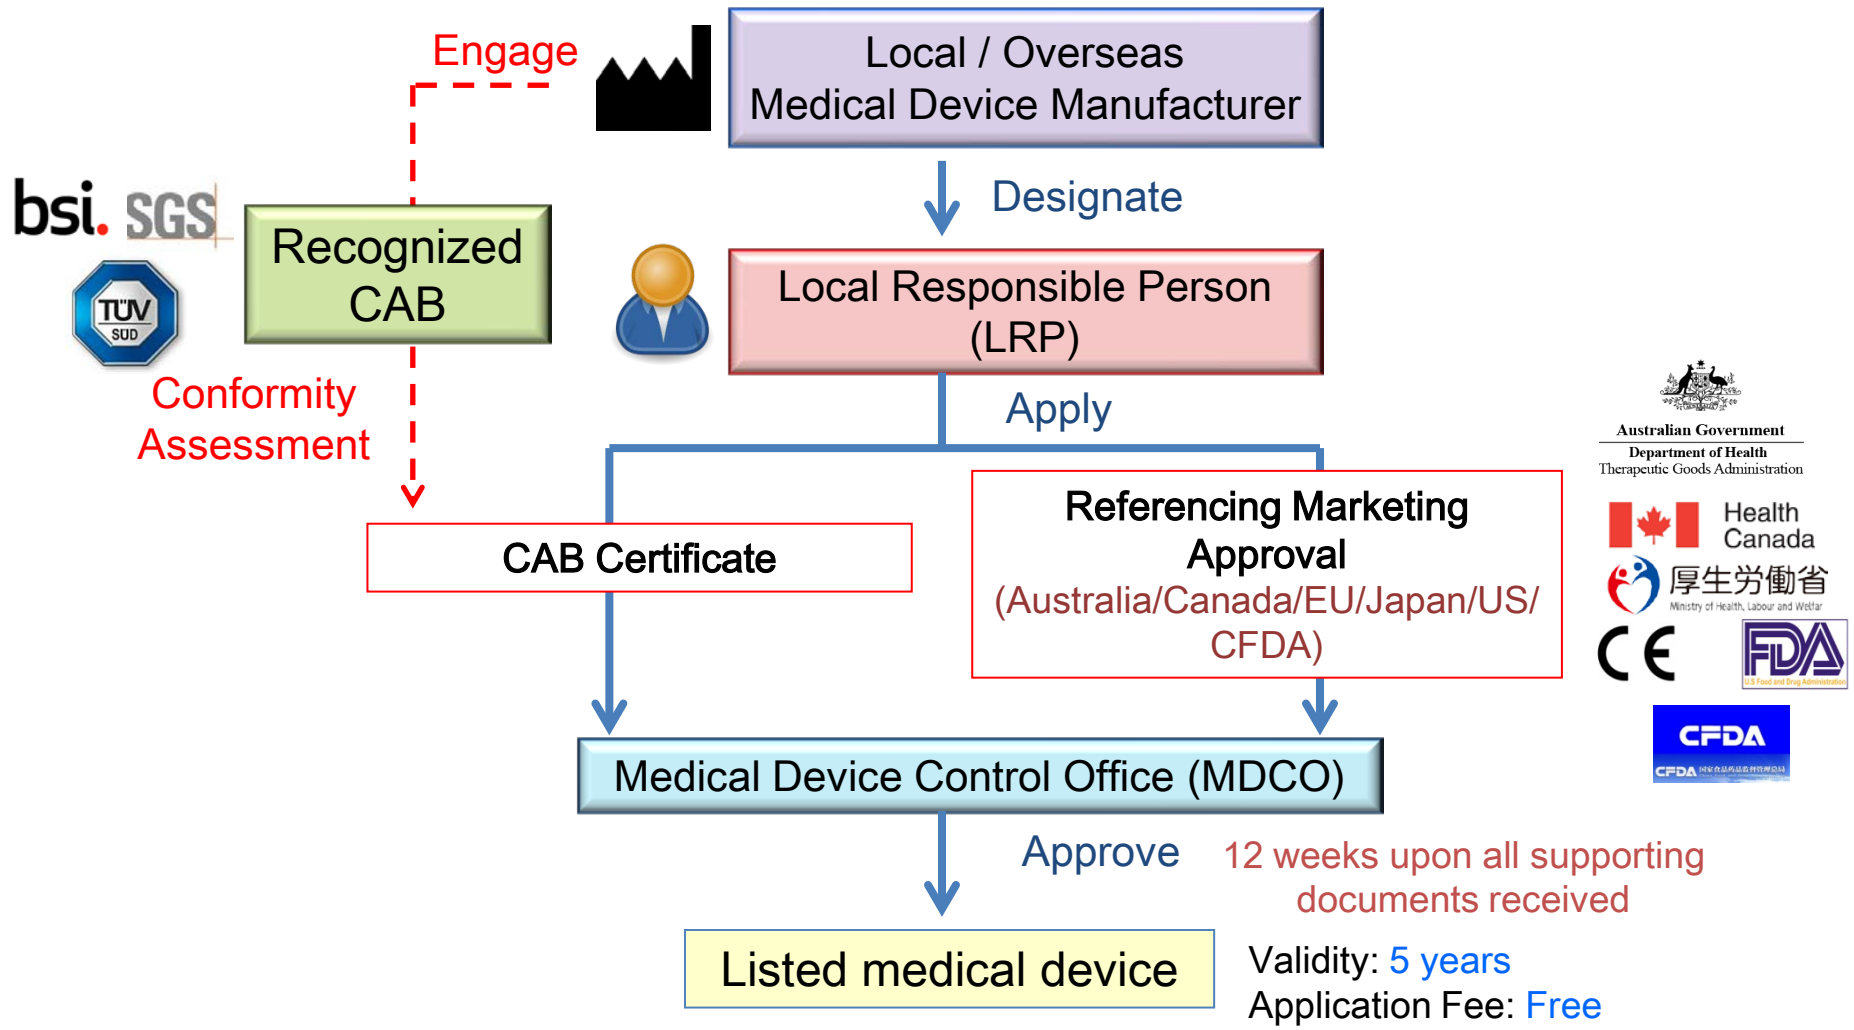



Listed Medical Device

Listed medical device (active) : 3 623[^]

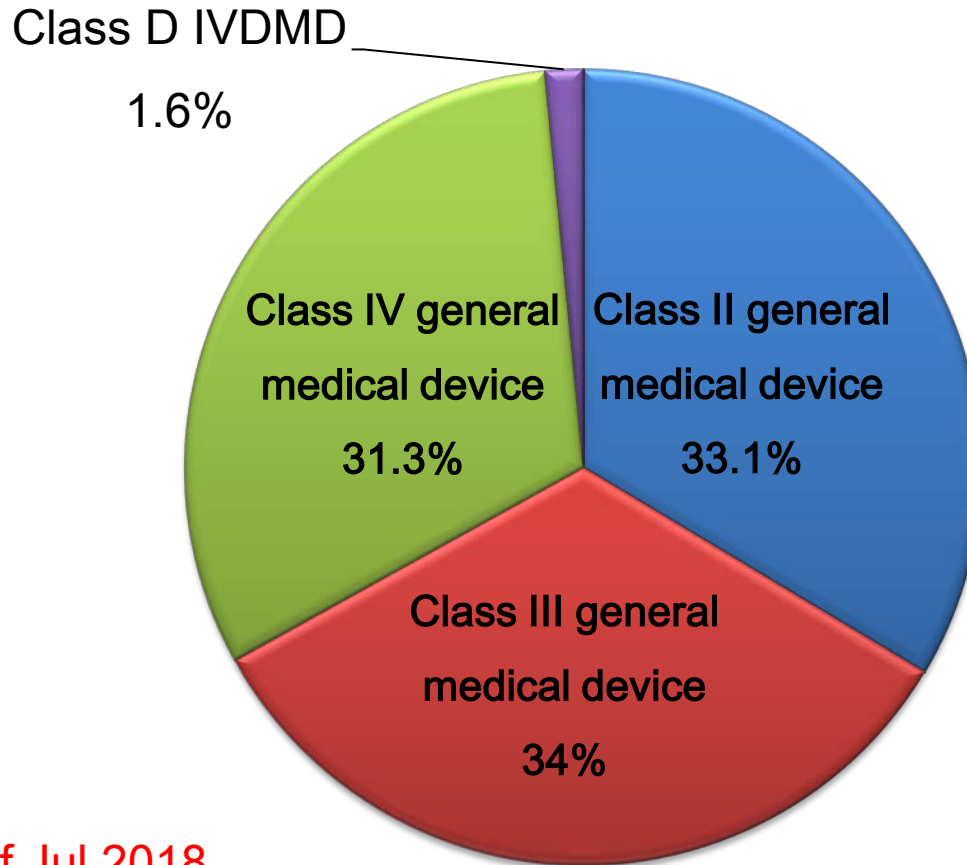

Note: [^] As of Jul 2018


Safety Alerts and Adverse Incidents Reporting



衛生署

Department of Health

Medical Device Safety Alert System

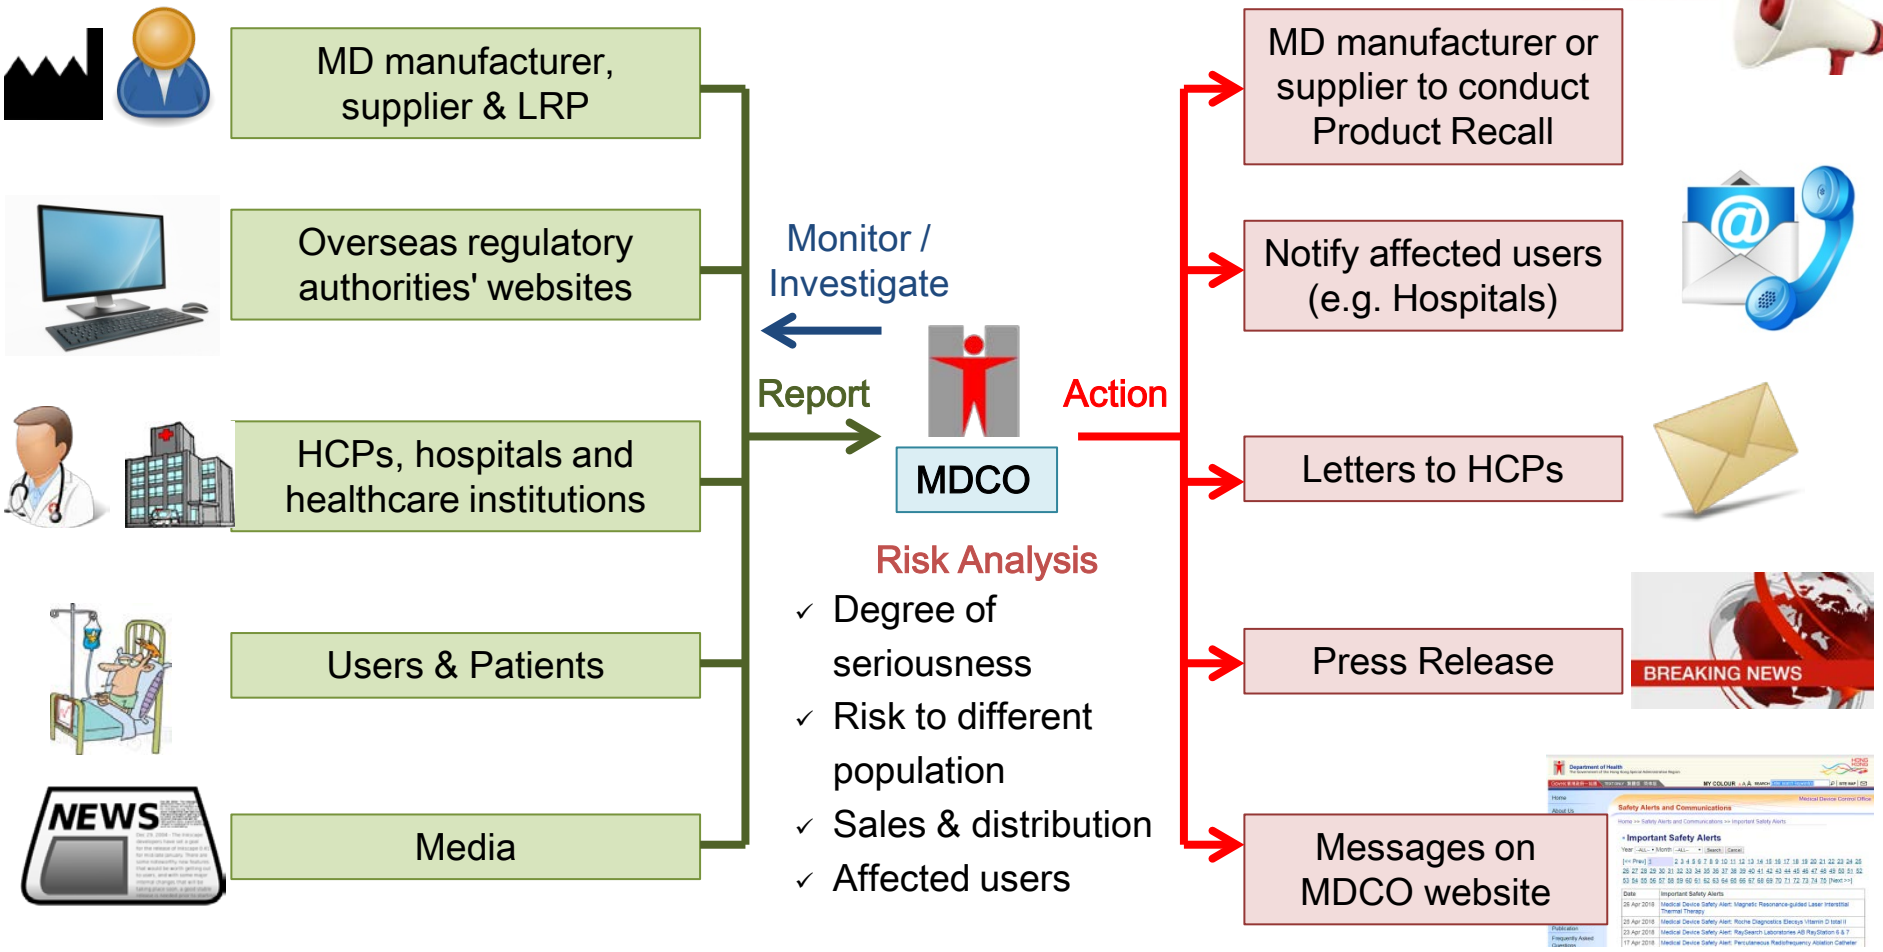


Adverse Incident Reporting



The Incident led to **one** of the following outcomes :

- ✓ Death of a patient, user or other person
- ✓ Serious injury of a patient, user or other person
- ✓ No death or serious injury occurred by the incident might lead to death or serious injury of a patient, user or other person if the incident recurs

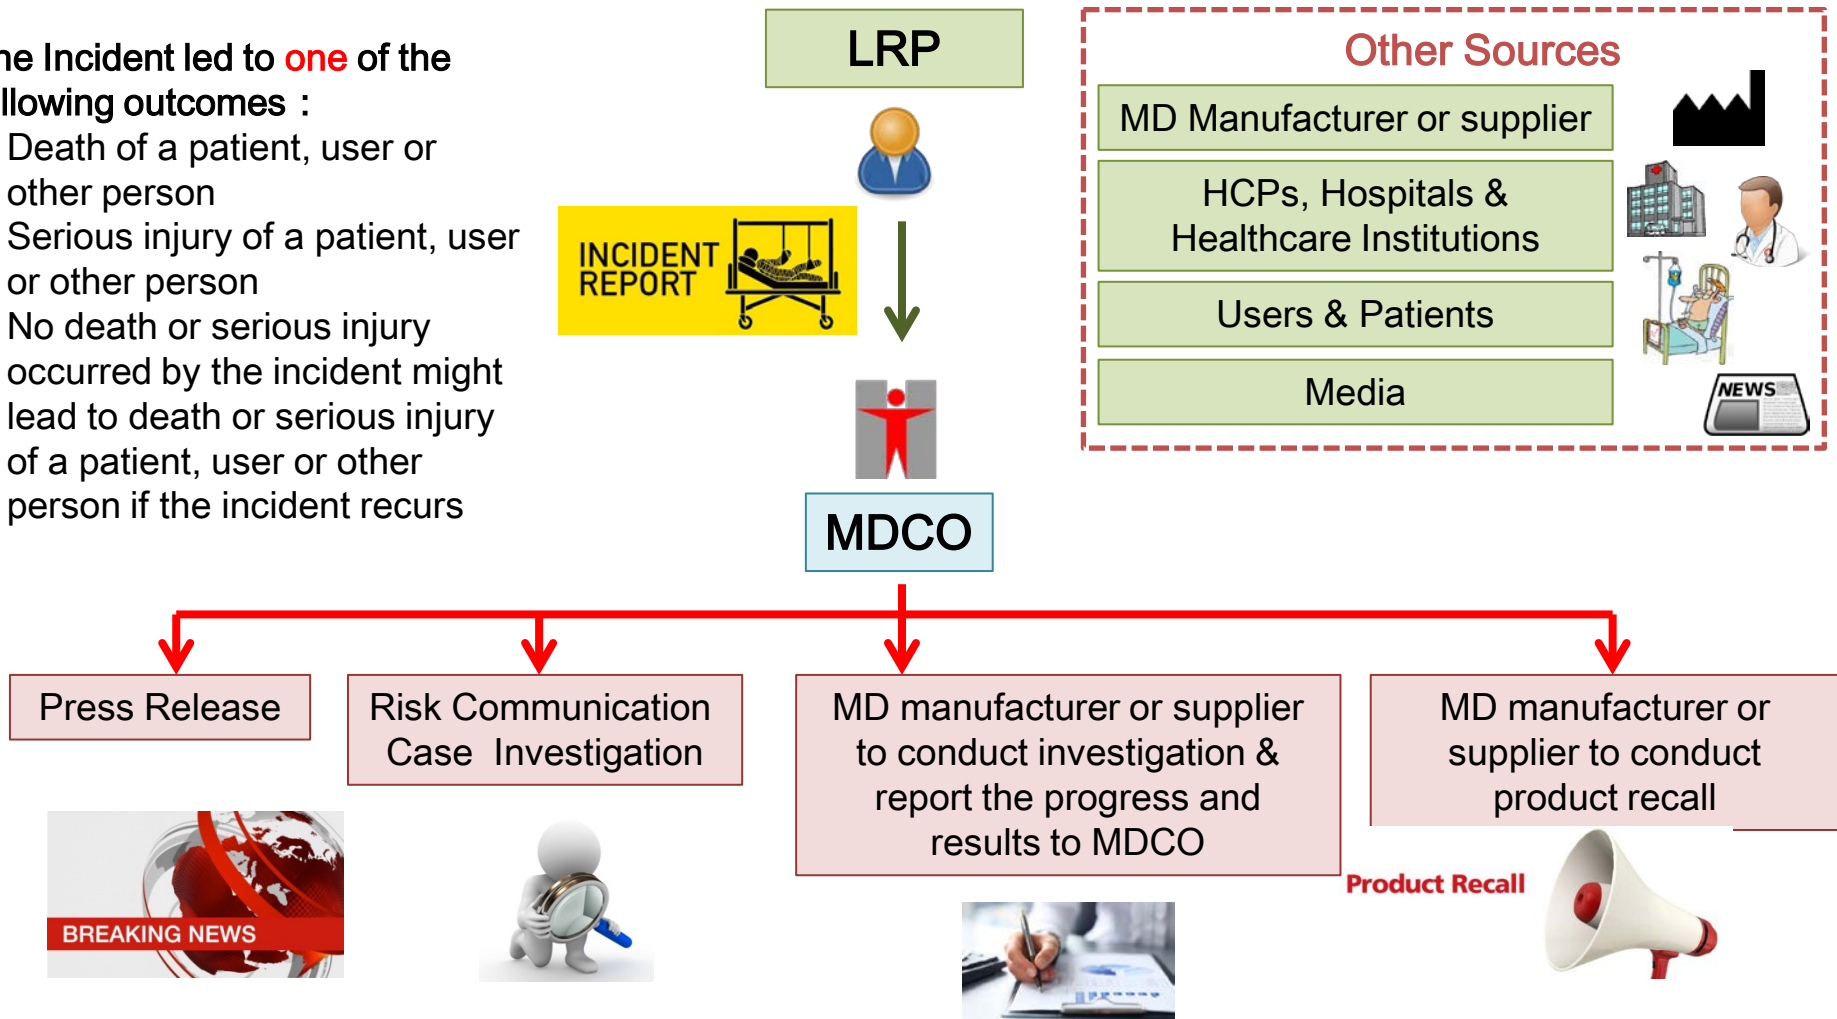

Useful Links



衛生署
Department of Health

■ Medical Device Control Office

www.mdco.gov.hk



◆ Issued Documents

(including Guidance Notes, Technical References, Code of Practice)

https://www.mdco.gov.hk/english/mdacs/mdacs_gn/mdacs_gn.html

◆ Search Database

(including List of Medical Devices, List of Traders & CABs)

<https://www.mdco.gov.hk/english/sd/sd.html>

◆ Information and Publication

(including pamphlet and Letters to Healthcare Professionals)

<https://www.mdco.gov.hk/english/emp/emp.html>

Thank you



衛生署

Department of Health